

# Anti-Prostate Specific Antigen antibody [EP1588Y] ab76113

**重组 RabMAb**

**11 References** [8 图像](#)

### 概述

<b>产品名称</b>	Anti-Prostate Specific Antigen抗体[EP1588Y]
<b>描述</b>	兔单克隆抗体[EP1588Y] to Prostate Specific Antigen
<b>宿主</b>	Rabbit
<b>特异性</b>	The antibody provided good results in western blot when tested in human prostate lysate. Unfortunately, when 22RV1 cell lysate was used no band was detected and inconsistent results were obtained with LNCaP cell lysate (where different lots of cell lysate were used for the test). Please contact our Scientific Support if you have any feedback and/or questions.
<b>经测试应用</b>	<b>适用于:</b> mIHC, WB, IHC-P
<b>种属反应性</b>	<b>与反应:</b> Human
<b>免疫原</b>	Synthetic peptide within Human Prostate Specific Antigen aa 200-300 (C terminal). The exact sequence is proprietary. Database link: <a href="#">P07288</a>
<b>阳性对照</b>	WB: LNCaP (Human prostate carcinoma epithelial cell) whole cell lysate and LNCaP (Human prostate carcinoma epithelial cell) treated with 100nM DHT for 2 days whole cell lysate IHC-P: Human prostate cancer tissue. mIHC: Human prostate gland tissues.
<b>常规说明</b>	This product is a recombinant monoclonal antibody, which offers several advantages including: <ul style="list-style-type: none"> <li>- High batch-to-batch consistency and reproducibility</li> <li>- Improved sensitivity and specificity</li> <li>- Long-term security of supply</li> <li>- Animal-free production</li> </ul> For more information <a href="#">see here</a> . Our RabMAb <sup>®</sup> technology is a patented hybridoma-based technology for making rabbit monoclonal antibodies. For details on our patents, please refer to <a href="#">RabMAb<sup>®</sup> patents</a> .  Mouse, Rat: We have preliminary internal testing data to indicate this antibody may not react with these species. Please contact us for more information.


### 性能

<b>形式</b>	Liquid
<b>存放说明</b>	Shipped at 4°C. Store at +4°C short term (1-2 weeks). Upon delivery aliquot. Store at -20°C long

term. Avoid freeze / thaw cycle.

### 解离常数 (K<sub>D</sub>)

K<sub>D</sub> = 5.04 x 10<sup>-10</sup> M

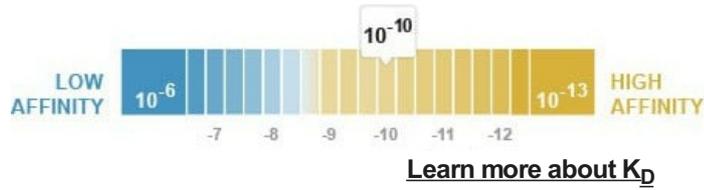

### 存储溶液

pH: 7.20  
 Preservative: 0.01% Sodium azide  
 Constituents: 59% PBS, 40% Glycerol (glycerin, glycerine), 0.05% BSA

### 纯度

Protein A purified

### 克隆

单克隆

### 克隆编号

EP1588Y

### 同种型

IgG

### 应用

**The Abpromise guarantee**      **Abpromise™**承诺保证使用ab76113于以下的经测试应用

“应用说明”部分 下显示的仅为推荐的起始稀释度;实际最佳的稀释度/浓度应由使用者检定。

应用	Ab评论	说明
mlHC		1/2000.
WB		1/1000. Detects a band of approximately 34 kDa (predicted molecular weight: 29 kDa). <b>For unpurified use at 1/10,000 - 1/50,000</b>
IHC-P		1/1000. Perform heat mediated antigen retrieval before commencing with IHC staining protocol. See <a href="#">IHC antigen retrieval protocols</a> . <b>For unpurified use at 1/100 - 1/250</b>


### 靶标

**功能**      Hydrolyzes semenogelin-1 thus leading to the liquefaction of the seminal coagulum.

**序列相似性**      Belongs to the peptidase S1 family. Kallikrein subfamily.  
Contains 1 peptidase S1 domain.


**细胞定位**      Secreted.

### 图片

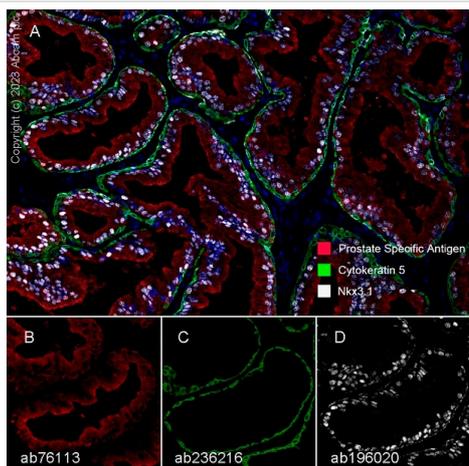

Multiplex immunohistochemistry - Anti-Prostate Specific Antigen antibody [EP1588Y] (ab76113)

Fluorescence multiplex immunohistochemical analysis of human prostate gland tissue (formalin/PFA-fixed paraffin-embedded section). Panel A: merged staining of anti-Prostate Specific Antigen (ab76113, red; Opal™690), anti-Cytokeratin 5 (ab236216, green; Opal™520) and anti-Nkx3.1 (ab196020, gray; Opal™570) on human prostate gland tissue. Panel B: anti-Prostate Specific Antigen stained on cytoplasm of luminal cells. Panel C: anti-Cytokeratin 5 stained on basal cells. Panel D: anti-p63 stained on nucleus of luminal cells. Opal Polymer HRP Ms + Rb was used as a secondary antibody. The immunostaining was performed on a Leica Biosystems BOND® RX instrument with an Opal™ 4-color kit. The section was incubated in three rounds of staining: in the order of ab76113 (1/2000), ab236216 (1/400) and ab196020 (1/2000) for 30 mins at room temperature. Each round was followed by a separate fluorescent tyramide signal amplification system. Each round was followed by a separate fluorescent tyramide signal amplification system. Heat mediated antigen retrieval with Tris-EDTA buffer (pH 9.0, epitope retrieval solution 2) was used for 20 mins. DAPI (blue) was used as a nuclear counter stain. Image acquisition was performed with Leica SP8 confocal microscope.

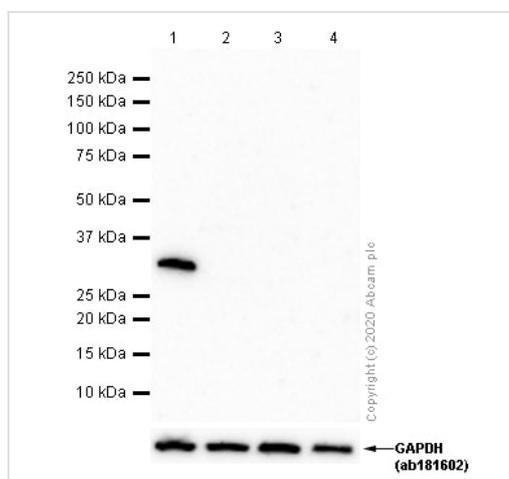

Western blot - Anti-Prostate Specific Antigen antibody [EP1588Y] (ab76113)

**All lanes :** Anti-Prostate Specific Antigen antibody [EP1588Y] (ab76113) at 1/1000 dilution ((Purified))

**Lane 1 :** LNCaP (Human prostate carcinoma epithelial cell) whole cell lysate at 15 µg

**Lane 2 :** PC-3 (Human prostate adenocarcinoma epithelial cell) whole cell lysate at 20 µg

**Lane 3 :** 22Rv1 (Human prostate carcinoma epithelial cell) whole cell lysate at 20 µg

**Lane 4 :** DU 145 (Human prostate carcinoma epithelial cell) whole cell lysate at 20 µg


### Secondary

**Lanes 1-3 :** Goat Anti-Rabbit IgG (HRP) with minimal cross-reactivity with human IgG at 1/2000 dilution

**Predicted band size:** 29 kDa

**Observed band size:** 34 kDa

The expression profile observed is consistent with what has been described in the literatures (PMID: 24906821, 17620434 and 25076860).

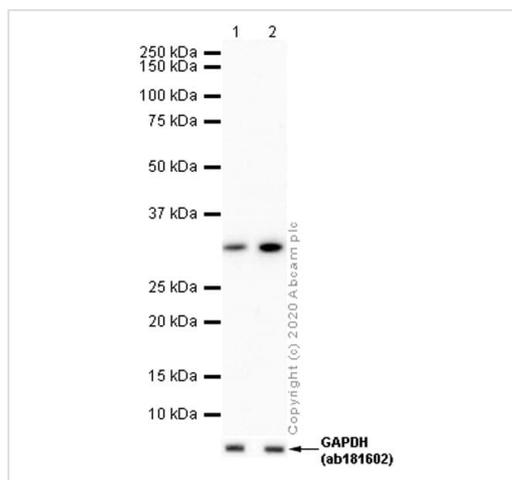

Western blot - Anti-Prostate Specific Antigen antibody [EP1588Y] (ab76113)

**All lanes** : Anti-Prostate Specific Antigen antibody [EP1588Y] (ab76113) at 1/1000 dilution

**Lane 1** : LNCaP (Human prostate carcinoma epithelial cell) whole cell lysate


**Lane 2** : LNCaP (Human prostate carcinoma epithelial cell) treated with 100nM DHT for 2 days whole cell lysate

Lysates/proteins at 15  $\mu$ g per lane.

### Secondary


**All lanes** : Goat Anti-Rabbit IgG H&L (HRP) ([ab97051](#)) at 1/20000 dilution

**Predicted band size:** 29 kDa

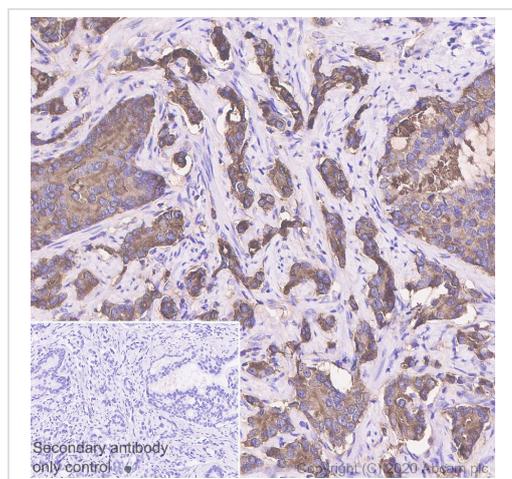


Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) - Anti-Prostate Specific Antigen antibody [EP1588Y] (ab76113)

Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) analysis of human prostate cancer tissue sections labeling Prostate Specific Antigen with purified ab76113 at 1/1000 dilution (0.51  $\mu$ g/mL). Heat mediated antigen retrieval using Bond™ Epitope Retrieval Solution 2 (pH 9.0). Rabbit specific IHC polymer detection kit HRP/DAB ([ab209101](#)) was used as the secondary antibody. Negative control: PBS instead of the primary antibody. Hematoxylin was used as a counterstain.

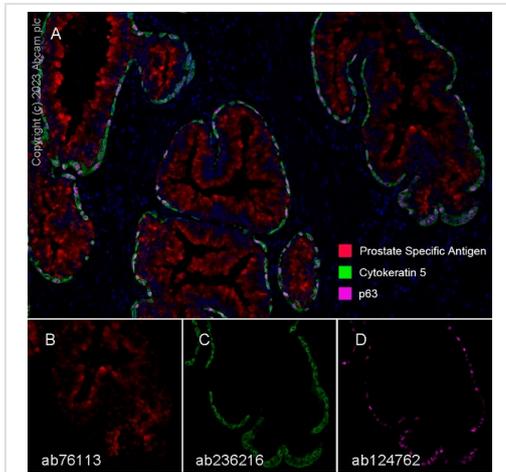

Multiplex immunohistochemistry - Anti-Prostate Specific Antigen antibody [EP1588Y] (ab76113)

Fluorescence multiplex immunohistochemical analysis of human prostate gland tissue (formalin/PFA-fixed paraffin-embedded section). Panel A: merged staining of anti-p63 ([ab124762](#), magenta; Opal™690), anti-Cytokeratin 5 ([ab236216](#), green; Opal™520) and anti-Prostate Specific Antigen (ab76113, red; Opal™570) on human prostate gland tissue. Panel B: anti-Prostate Specific Antigen stained on luminal cells. Panel C: anti-Cytokeratin 5 stained on cytoplasm of basal cells. Panel D: anti-p63 stained on nucleus of basal cells. Opal Polymer HRP Ms + Rb was used as a secondary antibody. The immunostaining was performed on a Leica Biosystems BOND® RX instrument with an Opal™ 4-color kit. The section was incubated in three rounds of staining: in the order of [ab124762](#) (1/5000), [ab236216](#) (1/400), and ab76113 (1/2000) for 30 mins at room temperature. Each round was followed by a separate fluorescent tyramide signal amplification system. Each round was followed by a separate fluorescent tyramide signal amplification system. Heat mediated antigen retrieval with Tris-EDTA buffer (pH 9.0, epitope retrieval solution 2) was used for 20 mins. DAPI (blue) was used as a nuclear counter stain. Image acquisition was performed with Leica SP8 confocal microscope.

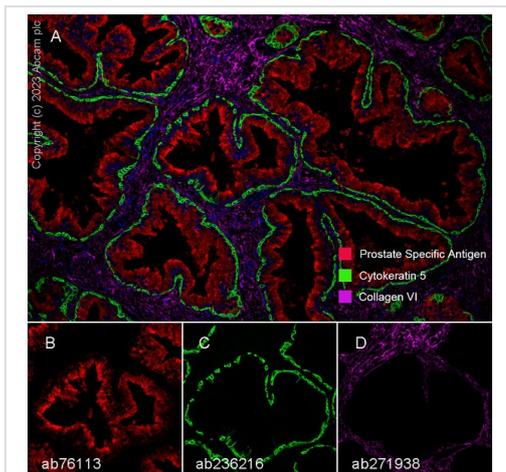

Multiplex immunohistochemistry - Anti-Prostate Specific Antigen antibody [EP1588Y] (ab76113)

Fluorescence multiplex immunohistochemical analysis of human prostate gland tissue (formalin/PFA-fixed paraffin-embedded section). Panel A: merged staining of anti-Collagen VI ([ab271938](#), magenta; Opal™690), anti-Cytokeratin 5 ([ab236216](#), green; Opal™520) and anti-Prostate Specific Antigen (ab76113, red; Opal™570) on human prostate gland tissue. Panel B: anti-Prostate Specific Antigen stained on luminal cells. Panel C: anti-Cytokeratin 5 stained on basal cells. Panel D: anti-Collagen VI stained on stroma. Opal Polymer HRP Ms + Rb was used as a secondary antibody. The immunostaining was performed on a Leica Biosystems BOND® RX instrument with an Opal™ 4-color kit. The section was incubated in three rounds of staining: in the order of [ab271938](#) (1/500), [ab236216](#) (1/400), and ab76113 (1/2000) for 30 mins at room temperature. Each round was followed by a separate fluorescent tyramide signal amplification system. Each round was followed by a separate fluorescent tyramide signal amplification system. Heat mediated antigen retrieval with Tris-EDTA buffer (pH 9.0, epitope

retrieval solution 2) was used for 20 mins. DAPI (blue) was used as a nuclear counter stain. Image acquisition was performed with Leica SP8 confocal microscope.

OI-RD Scanning - Anti-Prostate Specific Antigen antibody [EP1588Y] (ab76113)

Equilibrium disassociation constant ( $K_D$ )

Learn more about  $K_D$

**[Click here to learn more about  \$K\_D\$](#)**

### Why choose a recombinant antibody?



**Research with confidence**  
Consistent and reproducible results



**Long-term and scalable supply**  
Recombinant technology



**Success from the first experiment**  
Confirmed specificity



**Ethical standards compliant**  
Animal-free production

Anti-Prostate Specific Antigen antibody [EP1588Y] (ab76113)

**Please note:** All products are "FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES"

### Our Abpromise to you: Quality guaranteed and expert technical support

- Replacement or refund for products not performing as stated on the datasheet
- Valid for 12 months from date of delivery
- Response to your inquiry within 24 hours
- We provide support in Chinese, English, French, German, Japanese and Spanish
- Extensive multi-media technical resources to help you
- We investigate all quality concerns to ensure our products perform to the highest standards

If the product does not perform as described on this datasheet, we will offer a refund or replacement. For full details of the Abpromise, please visit <https://www.abcam.cn/abpromise> or contact our technical team.

### Terms and conditions

- Guarantee only valid for products bought direct from Abcam or one of our authorized distributors