


Anti-RPL7 antibody ab72550

★★★★★ [1 Abreviews](#) [23 References](#) [5 图像](#)

概述

产品名称	Anti-RPL7抗体
描述	兔多克隆抗体to RPL7
宿主	Rabbit
经测试应用	适用于: ICC/IF, WB, IP, IHC-P
种属反应性	与反应: Mouse, Human 预测可用于: Rat, Rabbit, Horse, Chicken, Guinea pig, Cow, Dog, Turkey, Pig, Rhesus monkey, Gorilla, Catfish, Orangutan, Xenopus tropicalis 
免疫原	Synthetic peptide corresponding to a region between residue 200 and the C-terminus (residue 248) of human RPL7 (NP_000962.2)
常规说明	<p>The Life Science industry has been in the grips of a reproducibility crisis for a number of years. Abcam is leading the way in addressing this with our range of recombinant monoclonal antibodies and knockout edited cell lines for gold-standard validation. Please check that this product meets your needs before purchasing.</p> <p>If you have any questions, special requirements or concerns, please send us an inquiry and/or contact our Support team ahead of purchase. Recommended alternatives for this product can be found below, along with publications, customer reviews and Q&As</p>

性能

形式	Liquid
存放说明	Shipped at 4°C. Upon delivery aliquot and store at -20°C. Avoid freeze / thaw cycles.
存储溶液	pH: 6.8 Preservative: 0.09% Sodium azide Constituents: 0.1% BSA, Tris buffered saline
纯度	Immunogen affinity purified
克隆	多克隆
同种型	IgG

应用

The Abpromise guarantee

Abpromise™ 承诺保证使用ab72550于以下的经测试应用

“应用说明”部分 下显示的仅为推荐的起始稀释度;实际最佳的稀释度/浓度应由使用者检定。

应用	Ab评论	说明
ICC/IF		Use at an assay dependent concentration.
WB	★★★★★ (1)	1/2000 - 1/10000. Detects a band of approximately 29 kDa (predicted molecular weight: 29 kDa).
IP		Use at 2-5 µg/mg of lysate.
IHC-P		Use a concentration of 1 mg/ml. Perform heat mediated antigen retrieval before commencing with IHC staining protocol.

靶标


功能

Binds to G-rich structures in 28S rRNA and in mRNAs. Plays a regulatory role in the translation apparatus; inhibits cell-free translation of mRNAs.

序列相似性

Belongs to the ribosomal protein L30P family.

图片

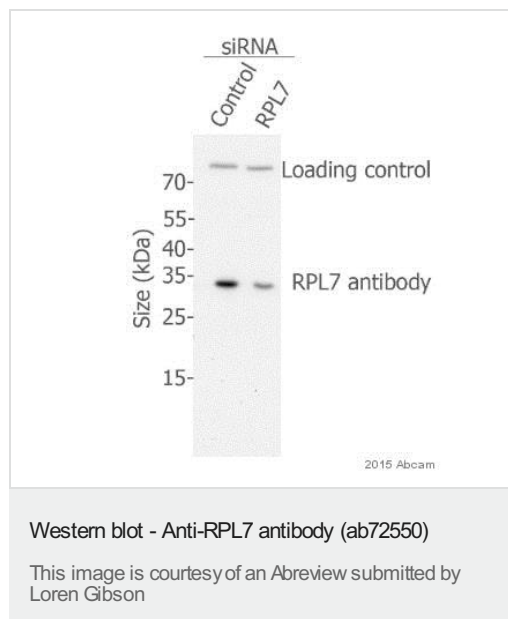

All lanes : Anti-RPL7 antibody (ab72550)

Lane 1 : U2OS whole cell lysate treated with control siRNA

Lane 2 : U2OS whole cell lysate treated with RPL7 siRNA

Lysates/proteins at 10 µg per lane.

Secondary

All lanes : HRP-conjugated donkey anti-rabbit IgG polyclonal at 1/1 dilution

Developed using the ECL technique.

Performed under reducing conditions.


Predicted band size: 29 kDa

Observed band size: 30 kDa

Exposure time: 10 seconds


Blocked with 2% milk for 1 hour at 18°C.

Incubated with the primary antibody in 2% milk for 18 hours at 4°C.

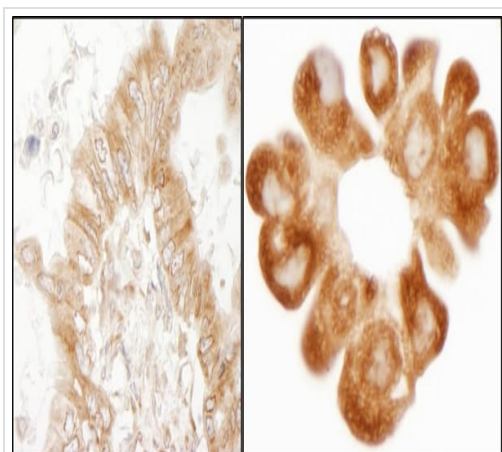

Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) - Anti-RPL7 antibody (ab72550)

Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) analysis of human lung carcinoma and bronchioalveolar carcinoma pleural effusion tissue labelling RPL7 with ab72550 at 1/1000 (0.2µg/ml) and 1/200 (1µg/ml). Detection: DAB.

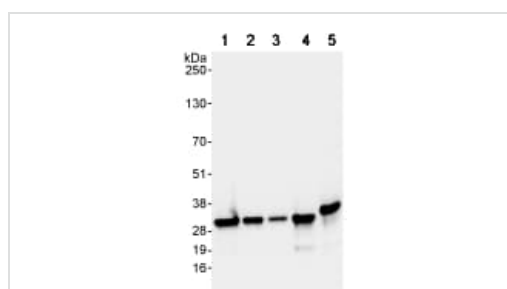

Western blot - Anti-RPL7 antibody (ab72550)

All lanes : Anti-RPL7 antibody (ab72550) at 0.04 µg/ml

Lane 1 : HeLa whole cell lysate at 50 µg

Lane 2 : HeLa whole cell lysate at 15 µg


Lane 3 : HeLa whole cell lysate at 5 µg

Lane 4 : 293T whole cell lysate at 50 µg

Lane 5 : NIH3T3 whole cell lysate at 50 µg


Predicted band size: 29 kDa

Observed band size: 29 kDa

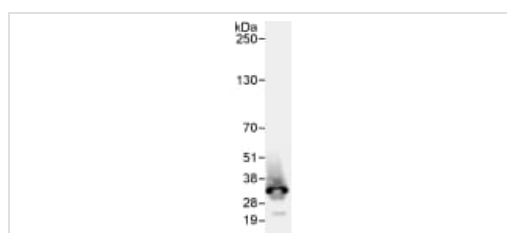

Immunoprecipitation - Anti-RPL7 antibody (ab72550)

Detection of Human RPL7 by Immunoprecipitation from Whole cell lysate from HeLa cells (1 mg for IP, 20% of IP loaded), using ab72550 at 3 µg/mg lysate for IP and at 1 µg/ml for subsequent Western blot detection.

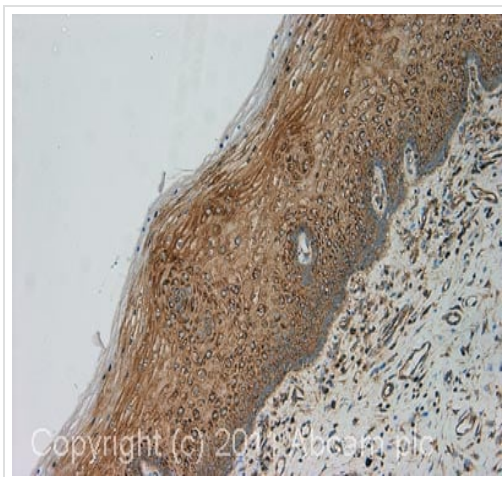

Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) - Anti-RPL7 antibody (ab72550)

IHC image of ab72550 staining in human normal cervix formalin fixed paraffin embedded tissue section, performed on a Leica Bond™ system using the standard protocol F. The section was pre-treated using heat mediated antigen retrieval with sodium citrate buffer (pH6, epitope retrieval solution 1) for 20 mins. The section was then incubated with ab72550, 1µg/ml, for 15 mins at room temperature and detected using an HRP conjugated compact polymer system. DAB was used as the chromogen. The section was then counterstained with haematoxylin and mounted with DPX.

For other IHC staining systems (automated and non-automated) customers should optimize variable parameters such as antigen retrieval conditions, primary antibody concentration and antibody incubation times.

Please note: All products are "FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES"

Our Abpromise to you: Quality guaranteed and expert technical support

- Replacement or refund for products not performing as stated on the datasheet
- Valid for 12 months from date of delivery
- Response to your inquiry within 24 hours
- We provide support in Chinese, English, French, German, Japanese and Spanish
- Extensive multi-media technical resources to help you
- We investigate all quality concerns to ensure our products perform to the highest standards

If the product does not perform as described on this datasheet, we will offer a refund or replacement. For full details of the Abpromise, please visit <https://www.abcam.cn/abpromise> or contact our technical team.

Terms and conditions

- Guarantee only valid for products bought direct from Abcam or one of our authorized distributors