

### Anti-FOXP3 antibody [mAbcam 450] ab450

★★★★★ [2 Abreviews](#) [23 References](#) [3 图像](#)

#### 概述

产品名称	Anti-FOXP3抗体[mAbcam 450]
描述	小鼠单克隆抗体[mAbcam 450] to FOXP3
宿主	Mouse
特异性	Detects a single clean band on human FOXP3 transfected 293 cells. When used in immunocytochemistry on acetone fixed FOXP protein transfected COS cells the antibody only detects FOXP3 and not FOXP1, FOXP2 or FOXP4.
经测试应用	<b>适用于:</b> IHC-Fr, IHC-P, WB
种属反应性	<b>与反应:</b> Human
免疫原	Synthetic peptide corresponding to Human FOXP3 aa 400 to the C-terminus conjugated to keyhole limpet haemocyanin. Database link: <a href="#">Q9BZS1</a> (Peptide available as <a href="#">ab16809</a> )
阳性对照	IHC-P: FFPE Human tonsil tissue sections. IHC-Fr: Human tonsil tissue sections.
常规说明	<p>This antibody clone is manufactured by Abcam. If you require a custom buffer formulation or conjugation for your experiments, please contact <a href="mailto:orders@abcam.com">orders@abcam.com</a>.</p> <p>The Life Science industry has been in the grips of a reproducibility crisis for a number of years. Abcam is leading the way in addressing this with our range of recombinant monoclonal antibodies and knockout edited cell lines for gold-standard validation. Please check that this product meets your needs before purchasing.</p> <p>If you have any questions, special requirements or concerns, please send us an inquiry and/or contact our Support team ahead of purchase. Recommended alternatives for this product can be found below, along with publications, customer reviews and Q&amp;As</p>

#### 性能

形式	Liquid
存放说明	Shipped at 4°C. Store at +4°C short term (1-2 weeks). Upon delivery aliquot. Store at -20°C or -80°C. Avoid freeze / thaw cycle.
存储溶液	pH: 7.40 Preservative: 0.02% Sodium azide Constituents: PBS, 6.97% L-Arginine

纯度	Protein A purified
克隆	单克隆
克隆编号	mAbcam 450
骨髓瘤	Sp2/0-Ag14
同种型	IgG3
轻链类型	kappa

## 应用

**The Abpromise guarantee**      **Abpromise™**承诺保证使用ab450于以下的经测试应用


“应用说明”部分 下显示的仅为推荐的起始稀释度;实际最佳的稀释度/浓度应由使用者检定。

应用	Ab评论	说明
IHC-Fr		Use a concentration of 5 µg/ml.
IHC-P	★★★★★ (1)	1/50. This clone has been tested against FOXP3 transfectants of COS-1 cells fixed with acetone and also works against formalin-fixed paraffin-embedded FOXP3 transfectants heat retrieved with pH9 Tris-EDTA buffer.It did not show positive staining with cryostat or paraffin-embedded human tonsil.
WB		Use a concentration of 1 µg/ml. Detects a band of approximately 48 kDa (predicted molecular weight: 48 kDa).

## 靶标

功能	Probable transcription factor. Plays a critical role in the control of immune response.
疾病相关	Defects in FOXP3 are the cause of immunodeficiency polyendocrinopathy, enteropathy, X-linked syndrome (IPEX) [MIM:304790]; also known as X-linked autoimmunity-immunodeficiency syndrome. IPEX is characterized by neonatal onset insulin-dependent diabetes mellitus, infections, secretory diarrhea, trombocytopenia, anemia and eczema. It is usually lethal in infancy.
序列相似性	Contains 1 C2H2-type zinc finger. Contains 1 fork-head DNA-binding domain.
细胞定位	Nucleus.

## 图片

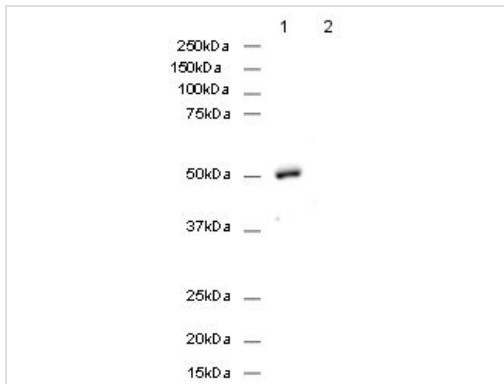

Western blot - Anti-FOXP3 antibody [mAbcam 450] (ab450)

**All lanes** : Anti-FOXP3 antibody [mAbcam 450] (ab450) at 1 µg/ml

**Lane 1** : HEK293 cells overexpressing human FOXP3

**Lane 2** : HEK293 cells overexpressing human FOXP3 with Human FOXP3 peptide ([ab16809](#)) at 1 µg/ml

Lysates/proteins at 20 µg per lane.


### Secondary

**All lanes** : Rabbit Anti-Mouse IgG H&L (HRP) ([ab6728](#)) at 1/5000 dilution

Performed under reducing conditions.

**Predicted band size:** 48 kDa

**Exposure time:** 45 seconds

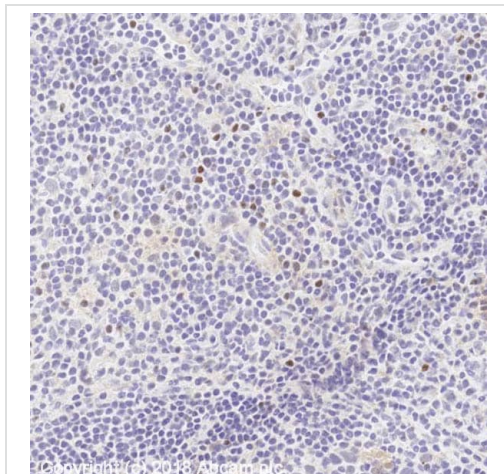


Immunohistochemistry (Frozen sections) - Anti-FOXP3 antibody [mAbcam 450] (ab450)

IHC image of FOXP3 staining in a section of formalin-fixed frozen normal human tonsil\* performed on a Leica BOND™ system using the standard protocol F. The section was then incubated with ab450, 5µg/ml, for 15 mins at room temperature and detected using an HRP conjugated compact polymer system. DAB was used as the chromogen. The section was then counterstained with haematoxylin and mounted with DPX.

For other IHC staining systems (automated and non-automated) customers should optimize variable parameters such as antigen retrieval conditions, primary antibody concentration and antibody incubation times.

*\*Tissue obtained from the Human Research Tissue Bank, supported by the NIHR Cambridge Biomedical Research Centre*

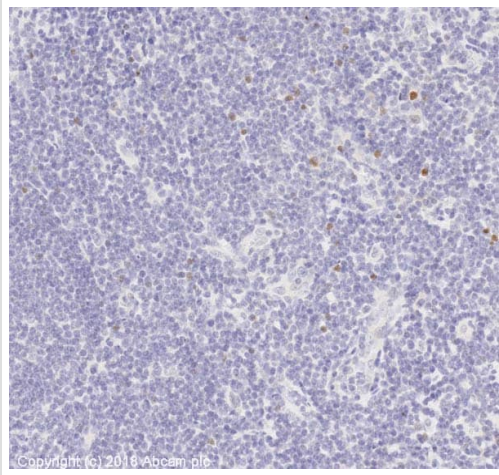

Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) - Anti-FOXP3 antibody [mAbcam 450] (ab450)

IHC image of FOXP3 staining in a section of formalin-fixed paraffin-embedded normal human tonsil\* performed on a Leica BOND™ system using the standard protocol F. The section was pre-treated using heat mediated antigen retrieval with sodium citrate buffer (pH6, epitope retrieval solution 1) for 20mins. The section was then incubated with ab450, 1ug/ml, for 15 mins at room temperature and detected using an HRP conjugated compact polymer system. DAB was used as the chromogen. The section was then counterstained with haematoxylin and mounted with DPX.

For other IHC staining systems (automated and non-automated) customers should optimize variable parameters such as antigen retrieval conditions, primary antibody concentration and antibody incubation times.

*\*Tissue obtained from the Human Research Tissue Bank, supported by the NIHR Cambridge Biomedical Research Centre*

**Please note:** All products are "FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES"

### Our Abpromise to you: Quality guaranteed and expert technical support

---

- Replacement or refund for products not performing as stated on the datasheet
- Valid for 12 months from date of delivery
- Response to your inquiry within 24 hours
- We provide support in Chinese, English, French, German, Japanese and Spanish
- Extensive multi-media technical resources to help you
- We investigate all quality concerns to ensure our products perform to the highest standards

If the product does not perform as described on this datasheet, we will offer a refund or replacement. For full details of the Abpromise, please visit <https://www.abcam.cn/abpromise> or contact our technical team.

### Terms and conditions

---

- Guarantee only valid for products bought direct from Abcam or one of our authorized distributors